



TRAINING HANDBOOK


Accu-Chek® Solo micropump system




ADJUSTING TIME BLOCKS

Editing a time block

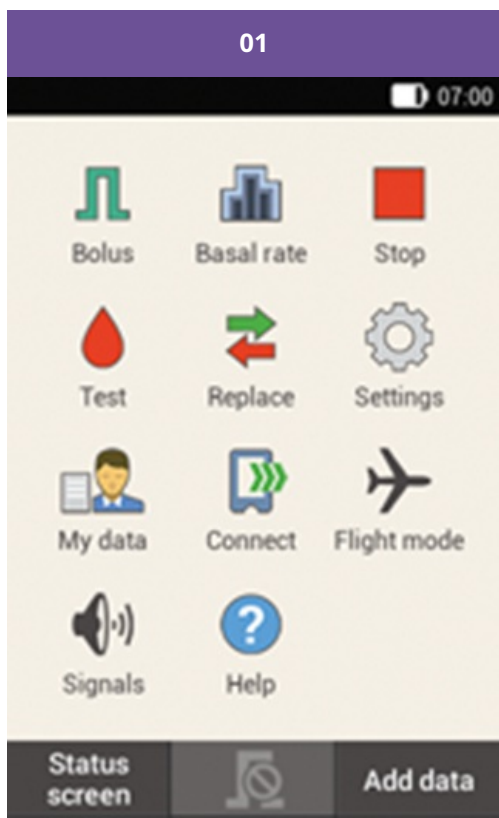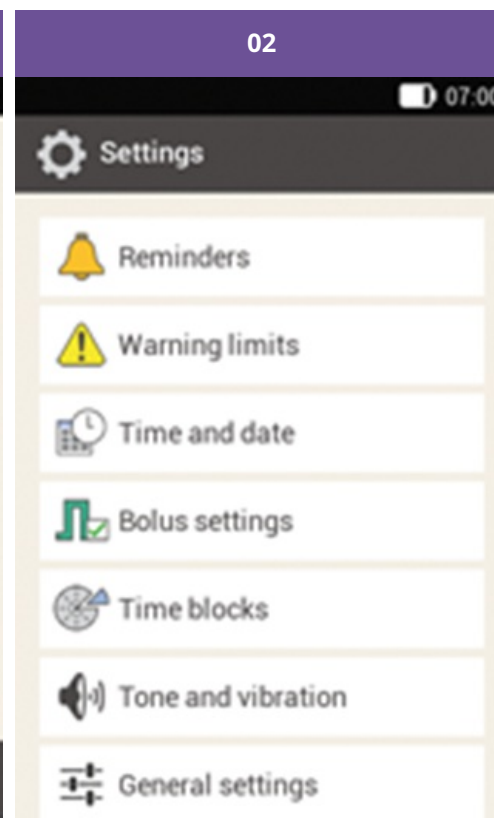 <p>01</p> <p>07:00</p> <p>Bolus Basal rate Stop</p> <p>Test Replace Settings</p> <p>My data Connect Flight mode</p> <p>Signals Help</p> <p>Status screen Add data</p>	 <p>02</p> <p>07:00</p> <p>Settings</p> <p>Reminders</p> <p>Warning limits</p> <p>Time and date</p> <p>Bolus settings</p> <p>Time blocks</p> <p>Tone and vibration</p> <p>General settings</p>
<p>In the Main menu, tap Settings.</p>	<p>Tap Time blocks.</p>

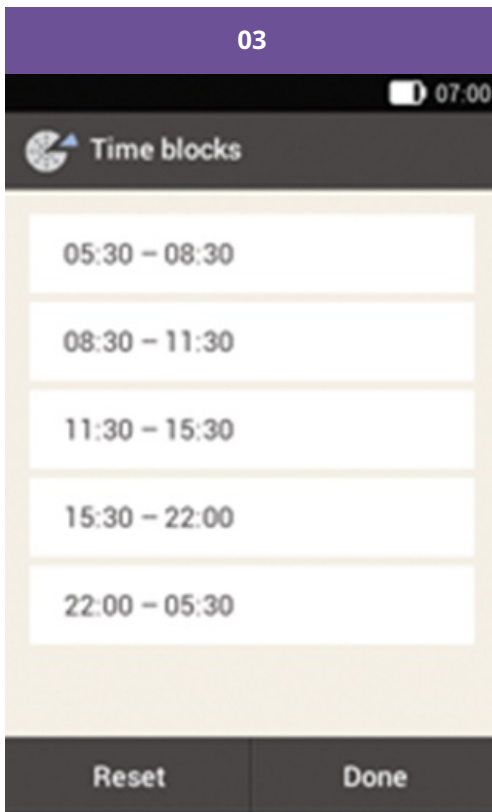


Tap the time block you want to edit.

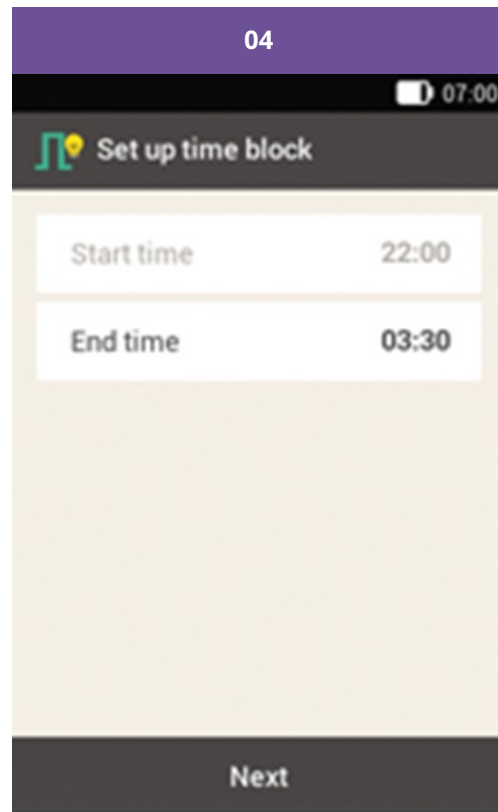


Adjust the end time.

Tap Next.

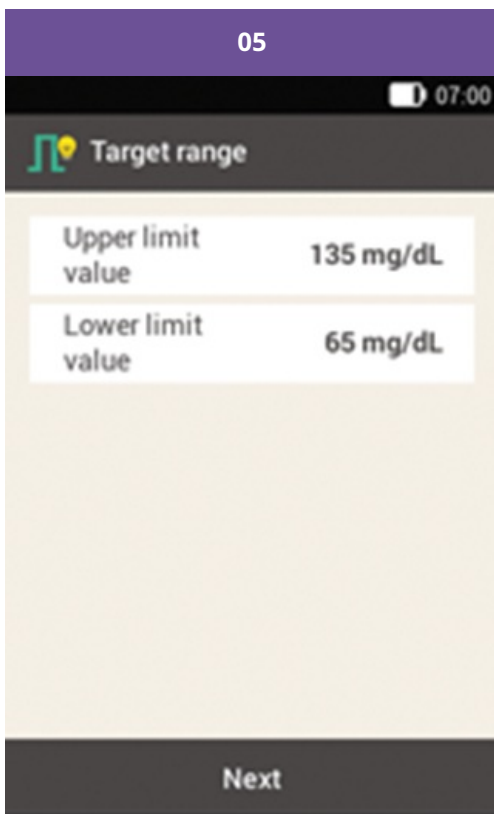


Adjust the upper limit value and lower limit value.

Tap [Next](#).

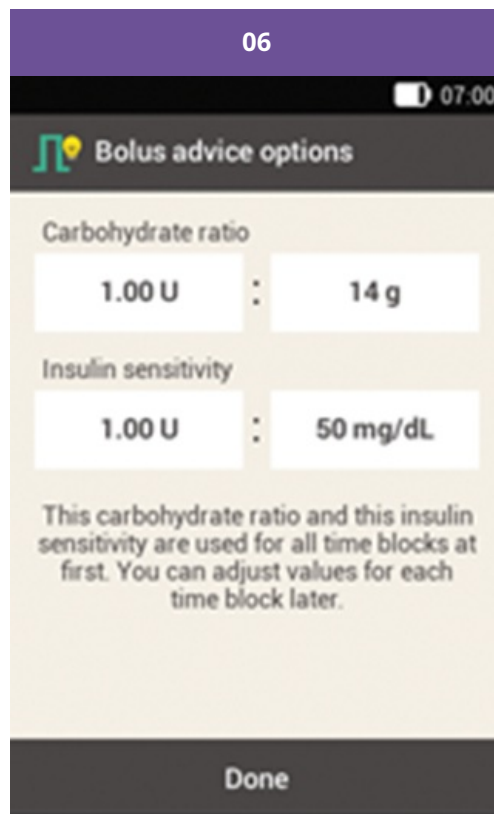

Adjust the carbohydrate ratio and insulin sensitivity.

Tap [Done](#).

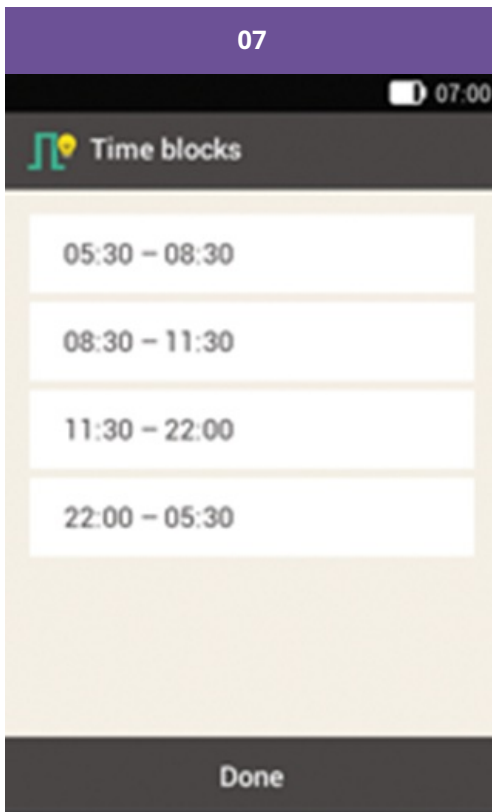


Once you have finished editing the time blocks, tap Done.

Adding a time block

This section describes how to add a new time block.


To add a time block, decrease the end time of the last time block.

After the new time block has been created, you may have to adjust the end time and other information for each time block.

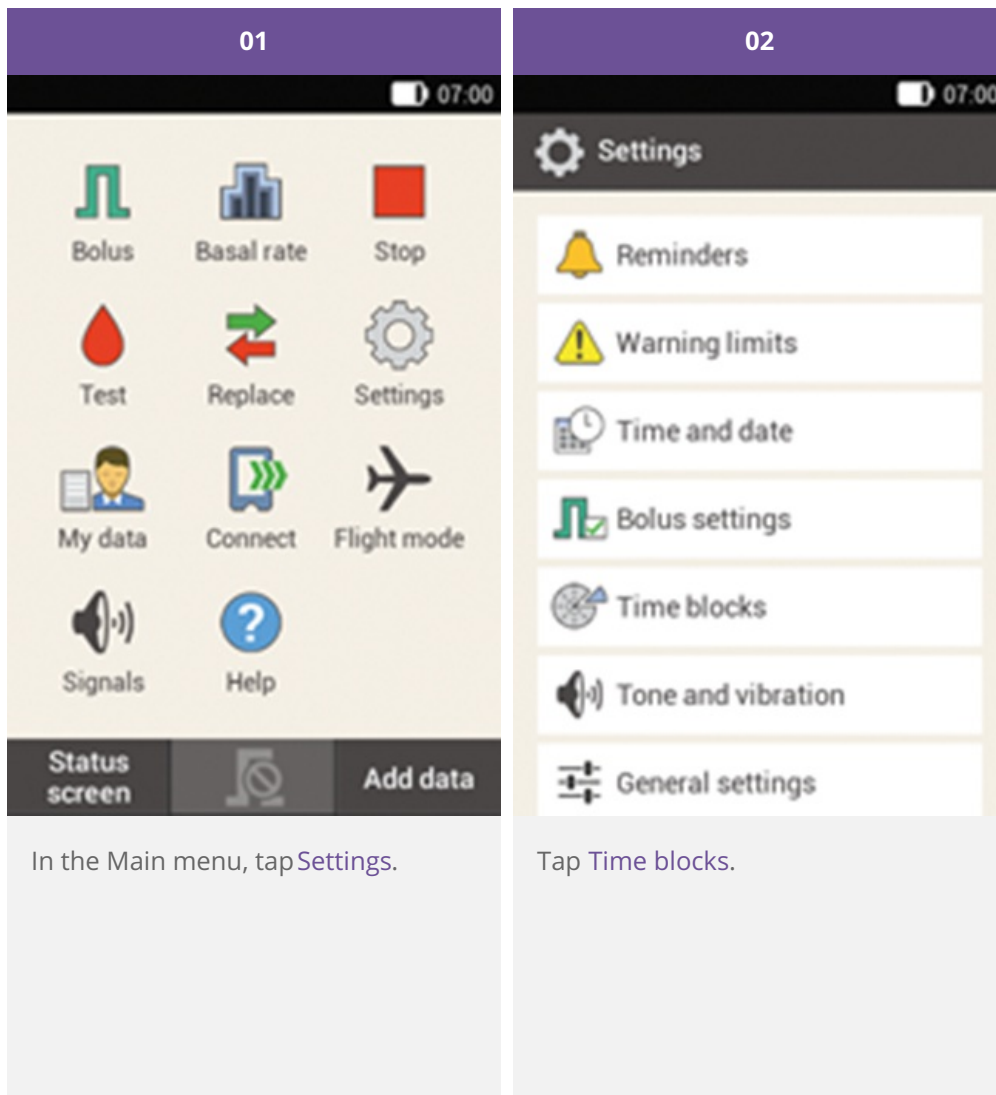




Tap the last time block.

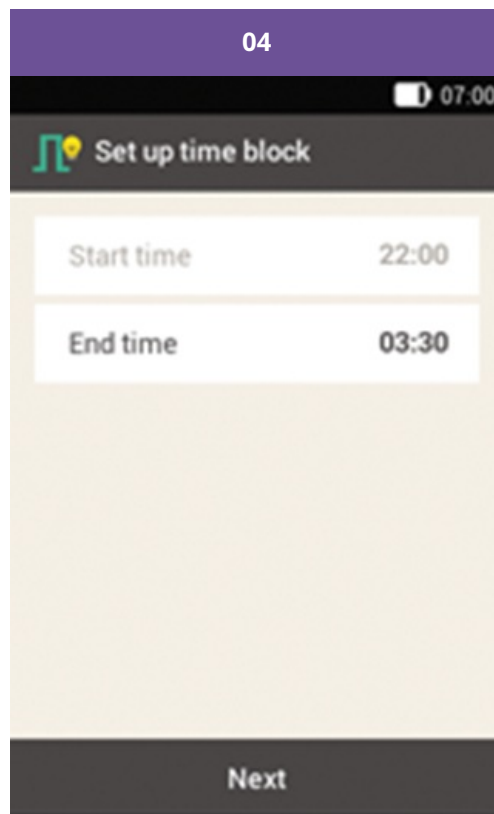


Tap End time and decrease the end time in order to create a new time block. However, do not decrease the end time until it equals the start time because this will delete the time block.

Tap Next.

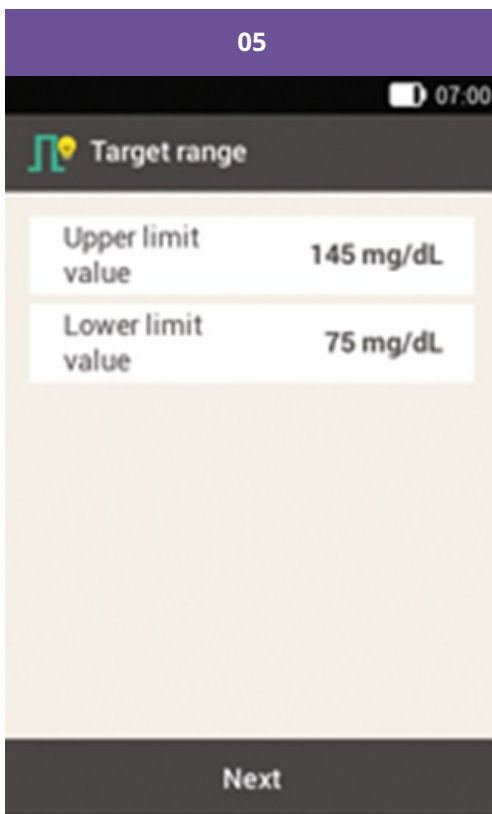


Set the upper limit value and lower limit value for the new time block.

Tap [Next](#).

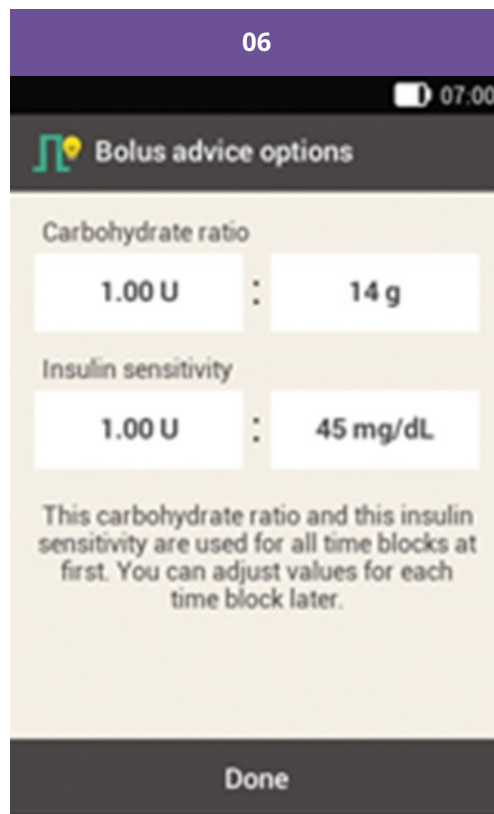

Set the carbohydrate ratio and insulin sensitivity for the new time block.

Tap [Done](#).

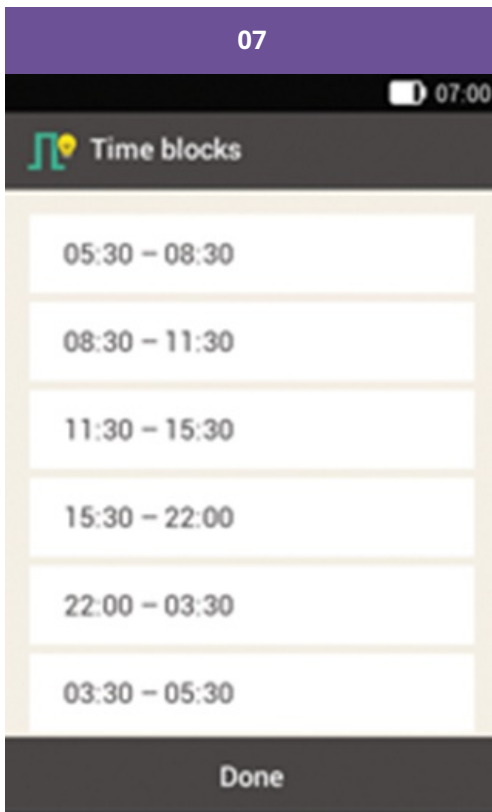


It may be necessary to change the end times and settings of other time blocks.


Tap **Done** when you have finished editing the time blocks.

Resetting all time blocks

This section describes how to restore the settings for all time blocks to the factory settings and then re-enter them.

Changing the start time of the first time block may be one reason for resetting all time blocks.

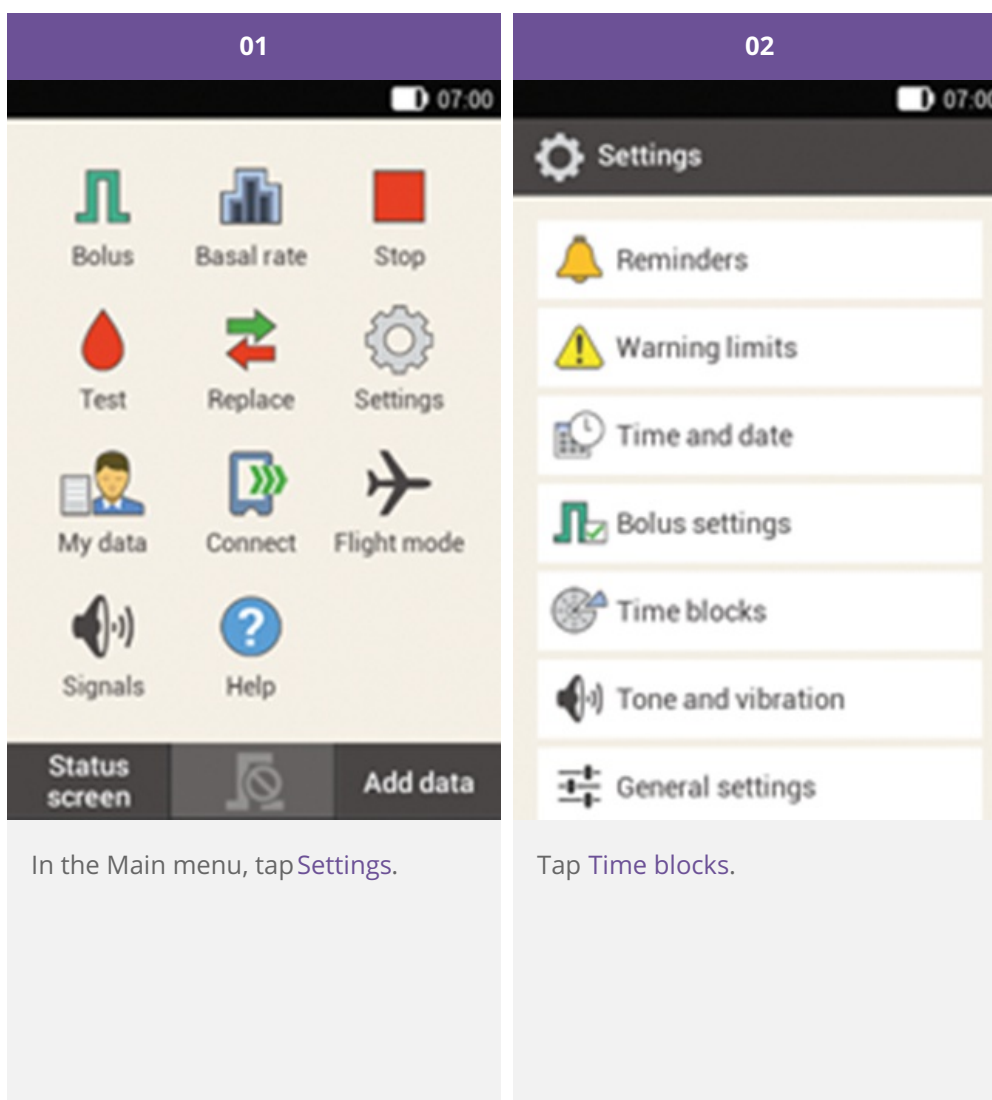


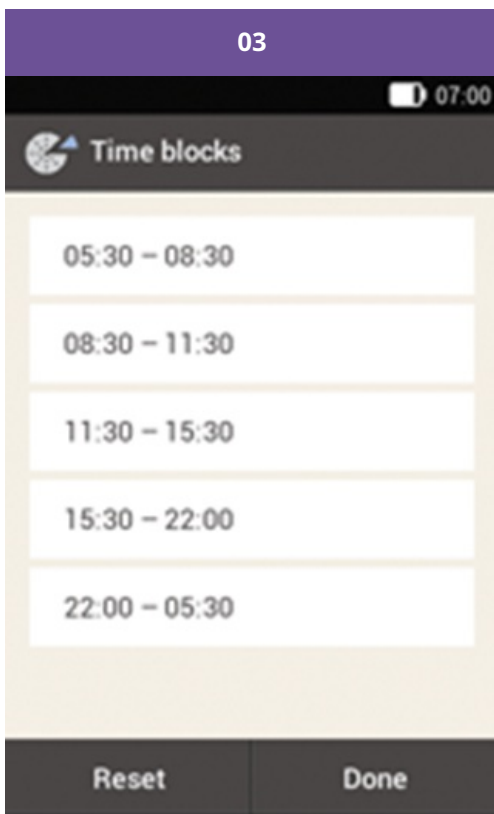

Tap [Reset](#).




If you want to reset all time blocks, tap [Yes](#).

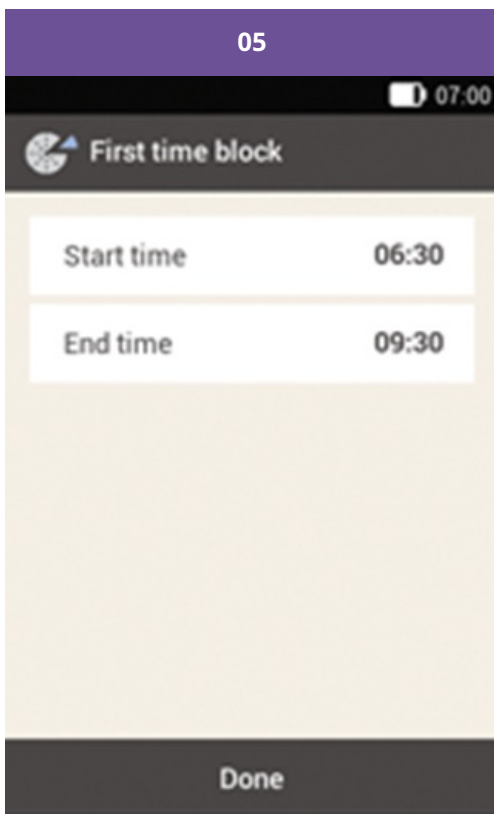


Set the start time and end time for the first time block.

Tap [Done](#).

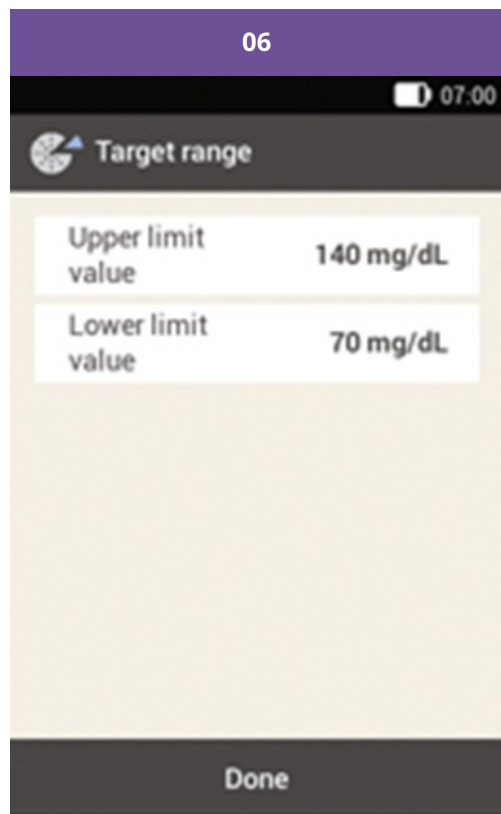

Set the default values for the upper limit value and lower limit value.

Tap [Done](#).

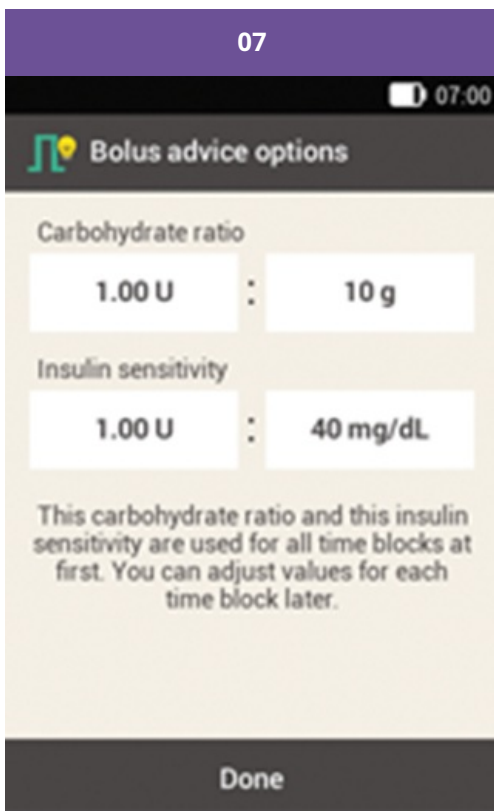


Set the default values for the carbohydrate ratio and insulin sensitivity.

Tap Done.



Tap OK.

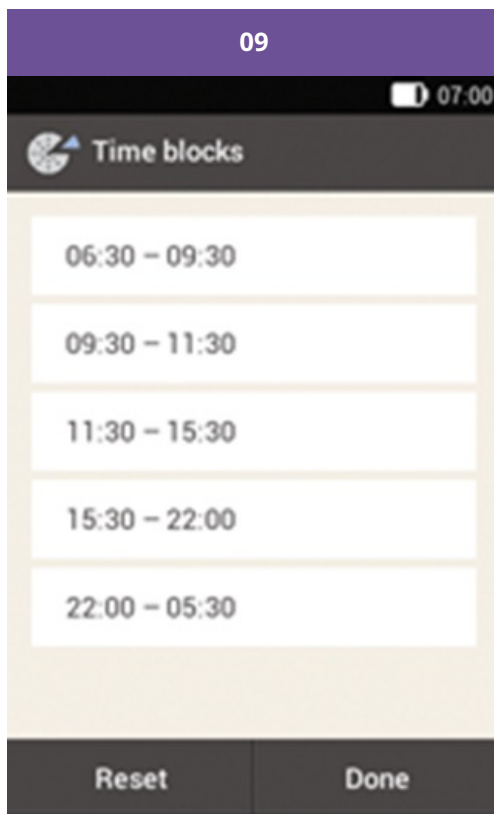

It may be necessary to change the end times and settings of the other time blocks.

Tap **Done** when you have finished editing the time blocks.

SETTINGS OVERVIEW

The Settings menu provides you with the following options to adjust the micropump system:

Setting	Explanation
Reminders	Help you to remember the tasks of your diabetes management. Reminders are explained separately in (Accu-Chek Solo micropump system) Chapter 14.2 .
Warning limits	Definition of limits for hyperglycemia (hyper) and hypoglycemia (hypo) and others.
Time and date	Setting the time and date correctly ensures that insulin is delivered at the right time of day.
Bolus settings	Parameter for bolus delivery and Quick bolus. For better overview, the Bolus Advice settings in this menu are explained in (Accu-Chek Solo micropump system) Chapter 9.4 .
Time blocks	Set start times, end times as well as target ranges, carb ratios and insulin sensitivities. With Bolus advice switched on, Time block settings can be found in the Bolus Advice menu. See (Accu-Chek Solo micropump system) Chapter 9.12 .
Tone and vibration	<ul style="list-style-type: none"> • Volume • Vibration • Tone for blood glucose test • System messages • Insulin delivery • Touchscreen setting • Signal suspension
General settings	<ul style="list-style-type: none"> • Language • Brightness • System function test
Screen lock	Protects your diabetes manager against accidental changes and entries.
System information	Technical information mainly used when communicating with pump support.
Injection mode	Mode for intensified conventional insulin therapy for which short-acting bolus insulin and long-acting basal insulin (depot insulin) is delivered using a syringe or pen.

 **Note**

When editing a setting, any unsaved changes are discarded once the diabetes manager turns off or a test strip is inserted into the test strip slot.

 **Warning**

The therapy settings must be provided by your healthcare professional and you may only change them after prior consultation. Using the wrong settings puts you at risk of hyper- or hypoglycemia.

Approved/listed/registered under the product name:
Accu-Chek Solo micropump system

ACCU-CHEK, ACCU-CHEK AVIVA, ACCU-CHEK AVIVA SOLO, ACCU-CHEK
SMART PIX,
ACCU-CHEK SOLO and FASTCLIX are trademarks of Roche.

The Bluetooth® word mark and logos are registered trademarks owned by
Bluetooth SIG,
Inc. and any use of such marks by Roche is under license.

All other product names and trademarks are the property of their
respective owners.

© 2021 Roche Diabetes Care

Roche Diabetes Care GmbH
Sandhofer Strasse 116
68305 Mannheim, Germany
www.accu-chek.com

