

TRAINING HANDBOOK

Accu-Chek® Solo micropump system





ADJUSTING AND ADDING BASAL RATE PROFILES

The reason behind different basal rate profiles

In addition to your initial basal profile, you may want to use other basal rate profiles for different daily routines. You can program up to 5 different basal profiles. Discuss using different basal profiles with your doctor or healthcare team.

Example

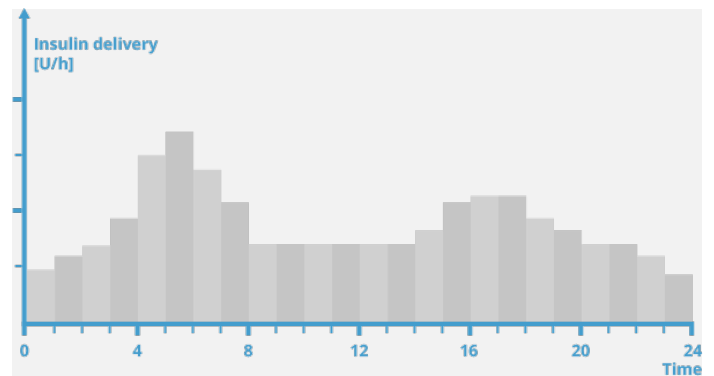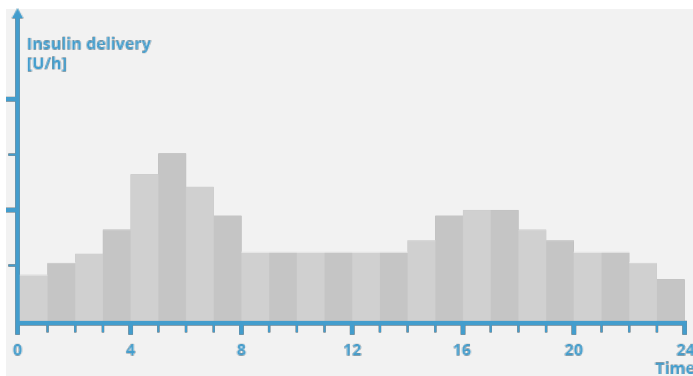



In this example, the user is a construction worker and from Monday to Friday he is on his feet from early morning until end of work. On the weekend, he likes to sleep in late and relax and read for hours. After discussing his varying daily routines with his doctor, the user programmed Basal Profile 1 for working days. He also programmed Basal Profile 2 that provides more basal insulin for Saturdays and Sundays.


Programming a basal rate profile

The image displays two screenshots of a mobile application interface for insulin management. The left screenshot shows the main menu with a glucose reading of 5.9 mmol/L, a bolus of 150 U, and a basal rate profile of 1.20 U/h. The right screenshot shows the status screen with a grid of icons for Bolus, Basal rate, Stop, Test, Replace, Settings, My data, Connect, Flight mode, Signals, and Help. Below the screenshots are instructions for navigating to the basal rate profile.


On the Status screen, tap the basal rate profile.

On the main menu, tap Basal rate.

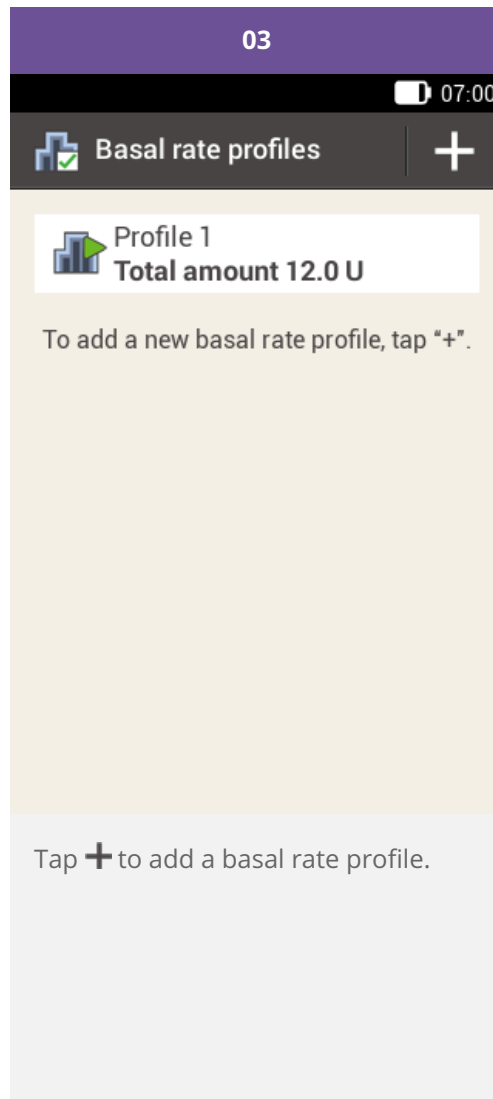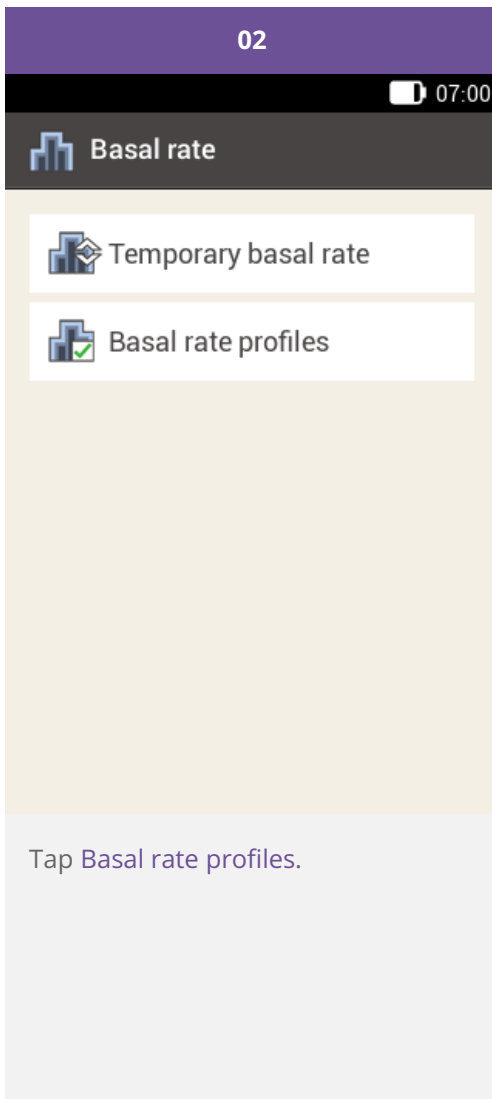

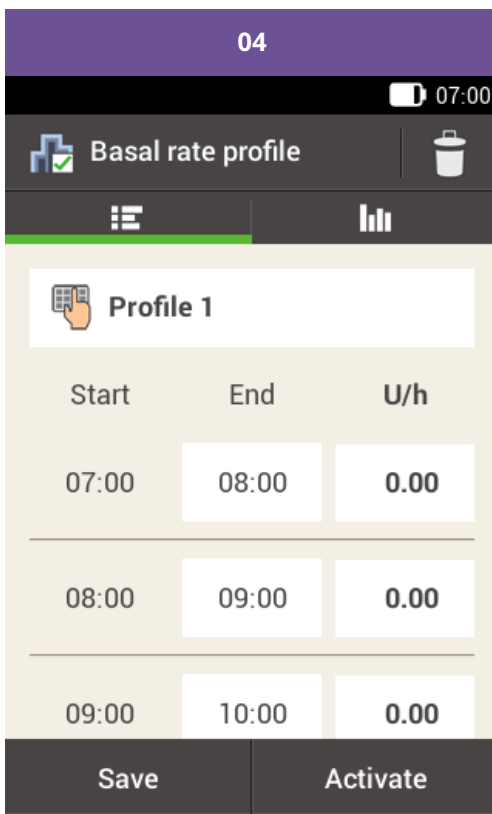


Tap to name the profile.

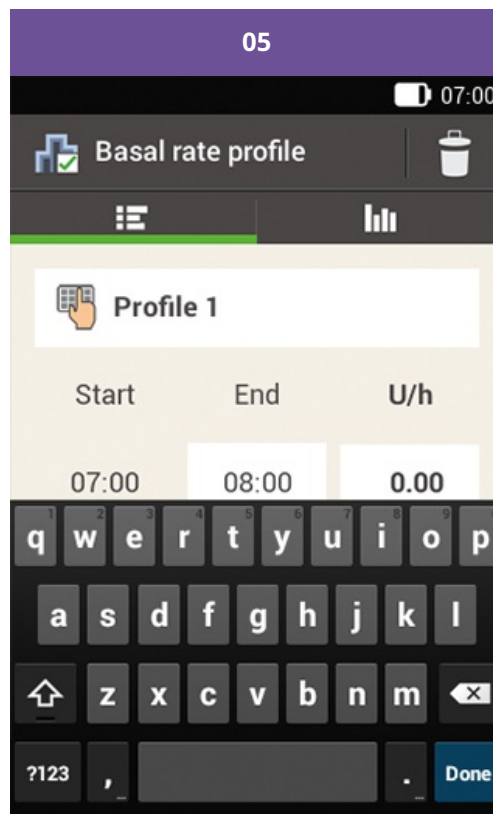


Enter the desired name for the basal rate profile (maximum 12 characters).

Then tap Done.

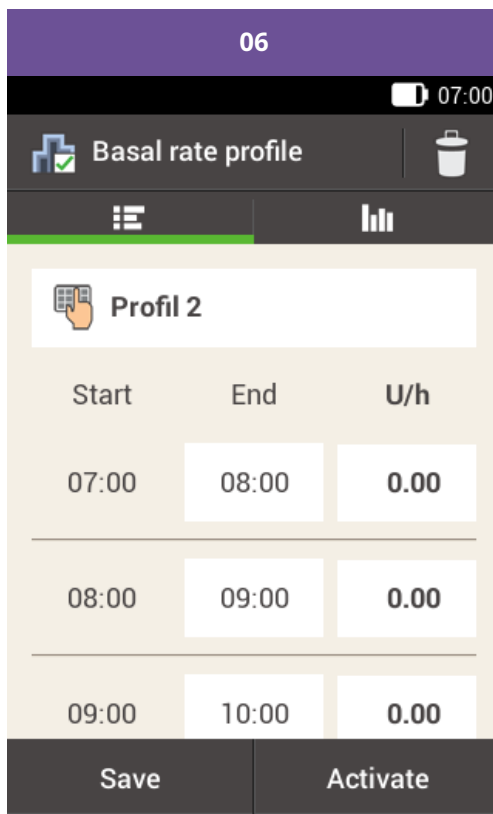

Select the first time block.

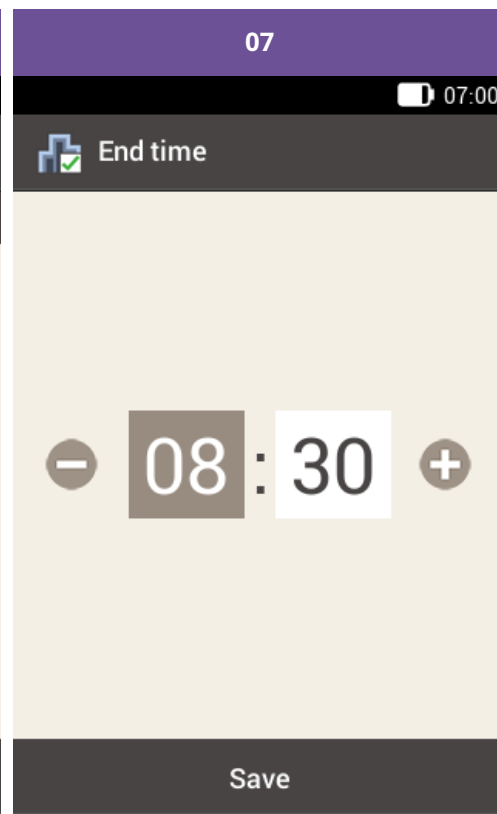

Enter the end time for the time block.

Tap Save.


Note

You are only able to edit the end time of basal rate time blocks. The start time of each time block is identical to the end time of the previous time block.

To delete a time block, set the end time of the time block to the start time of the same time block.

To add a new time block, set the end time of the last time block to the desired start time for the new time block.

Basal rate time blocks are neither identical to, nor shared with the time blocks for Bolus advice.

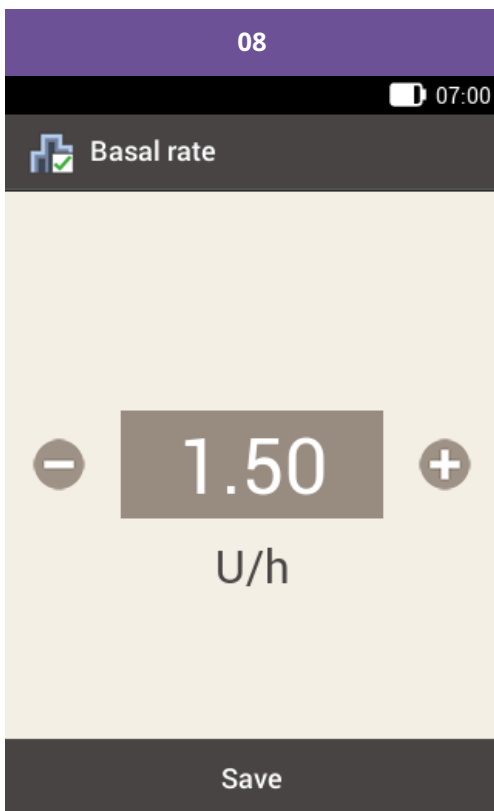


Enter the insulin amount per hour for the time block.

Tap [Save](#).


Continue to enter the end times and hourly basal rates until you have programmed the appropriate hourly basal rates for all 24 hours of the day.

If you wish to save but not currently activate this basal rate profile continue with step 09.

If you wish to save and activate the new basal profile immediately, tap "Activate". Continue with step 11.

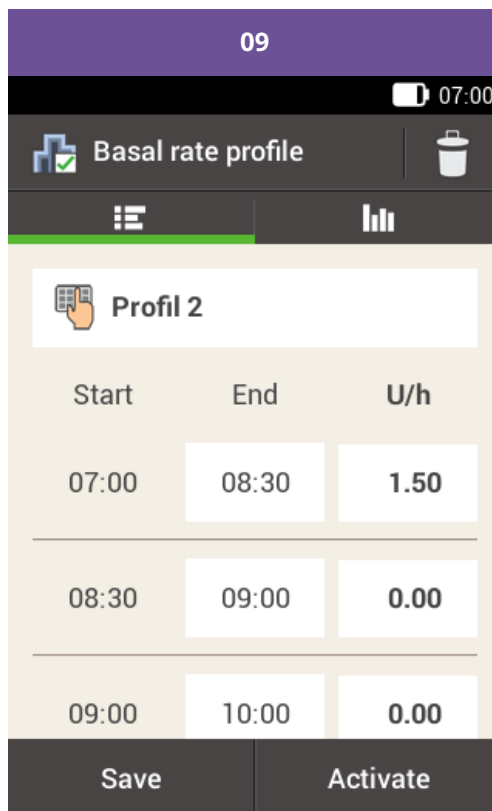

Tap [Save](#) to save the programmed Basal rate profile.

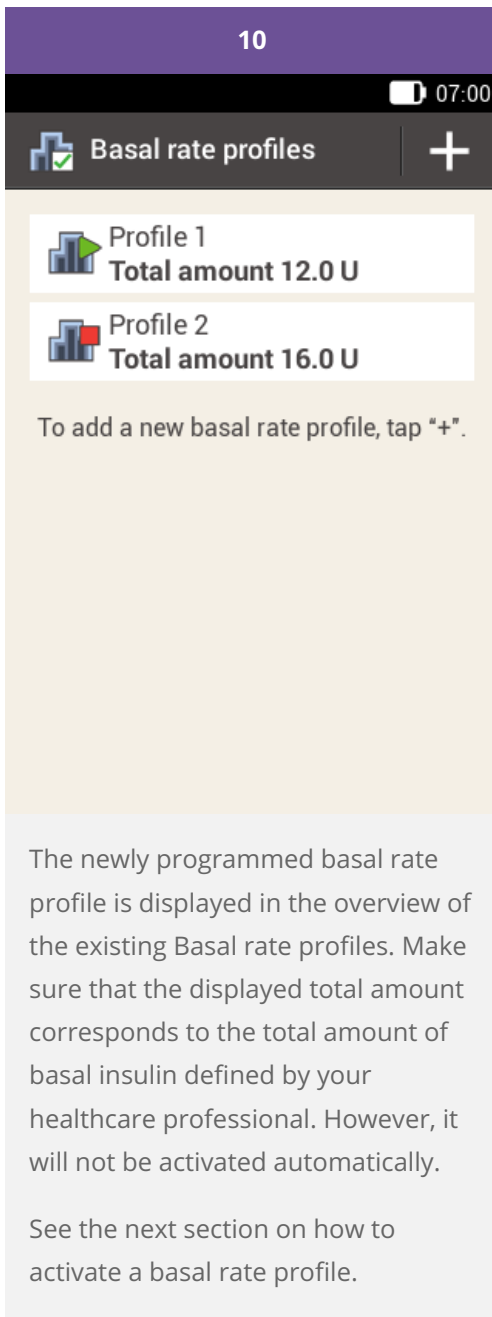

Activating a basal rate profile

Activate the appropriate profile, when it is due. For example, Friday night, when you change to your weekend routines, activate the profile you have programmed for weekends.

01

07:00

5.9 mmol/L
06:55, 29 Mar 2018

150 U

Profile 1
1.20 U/h

New bolus

Main menu **Add data**

07:00

Bolus Basal rate Stop

Test Replace Settings



My data Connect Flight mode


Signals Help

Status screen **Add data**


On the Status screen, tap the basal rate profile.

On the main menu, tap Basal rate.

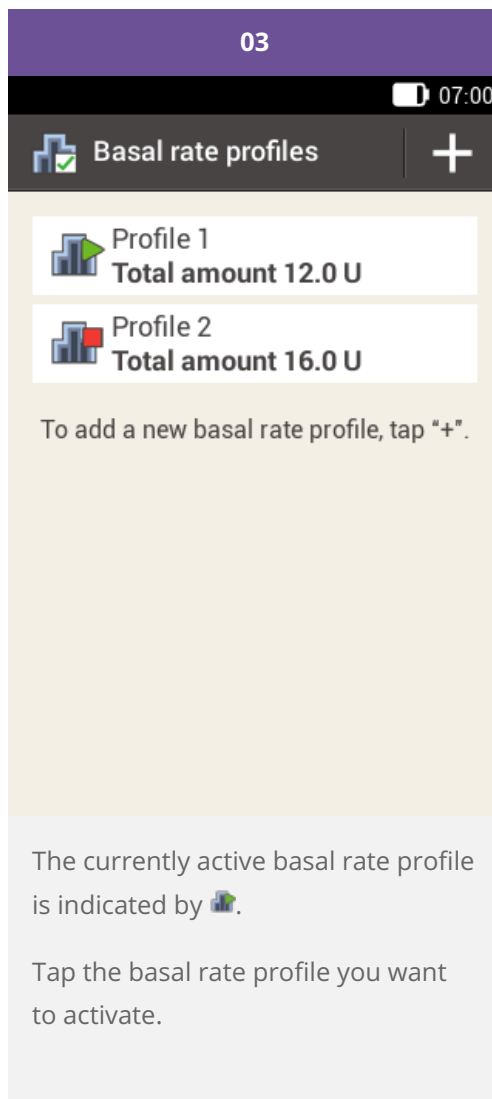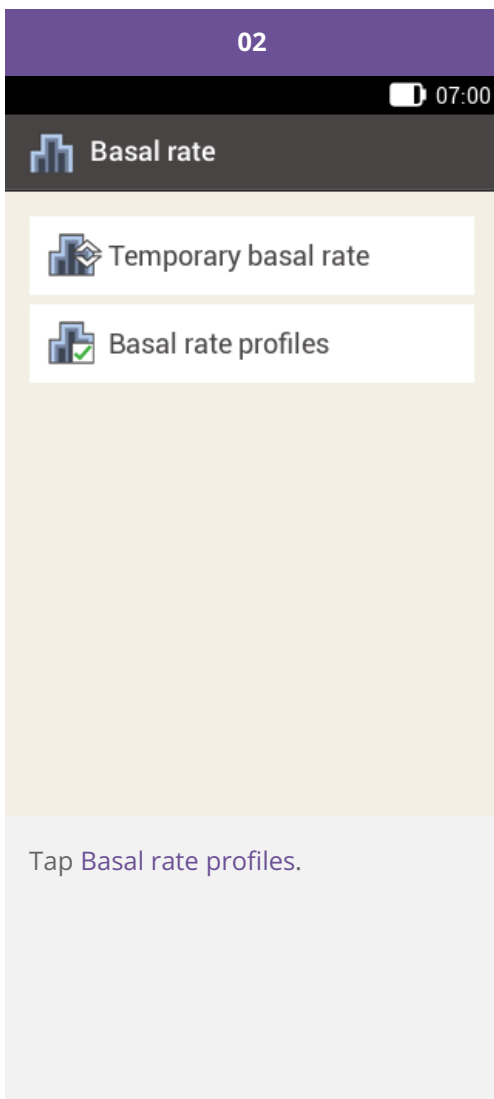


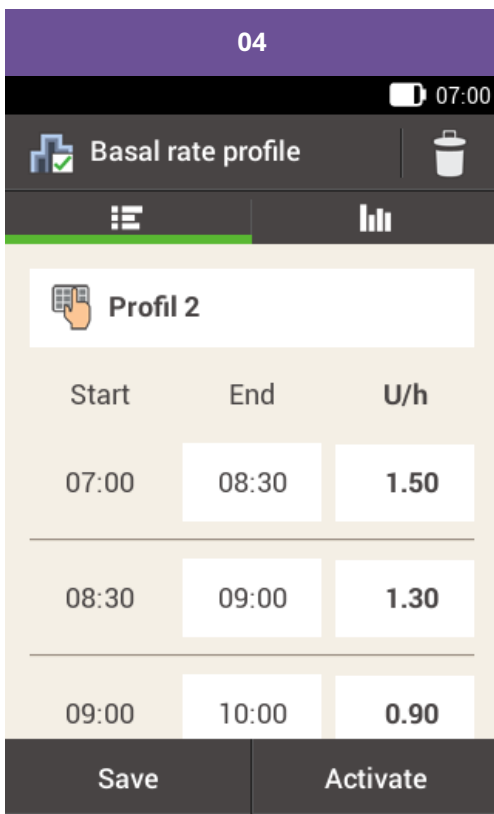


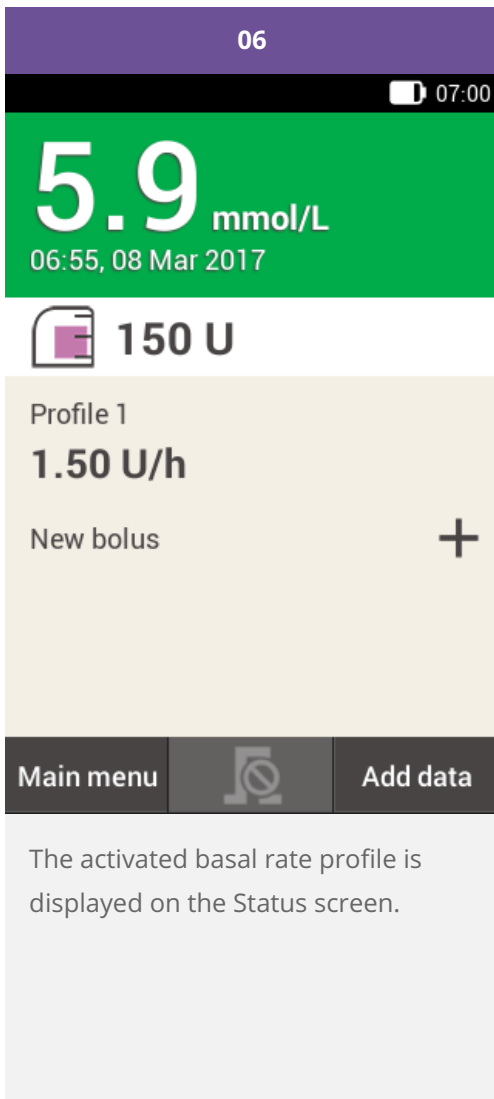
If required, scroll the screen upwards to see all time blocks of the basal rate profile.

Tap  to see the graphic for the profile.

Tap [Activate](#).

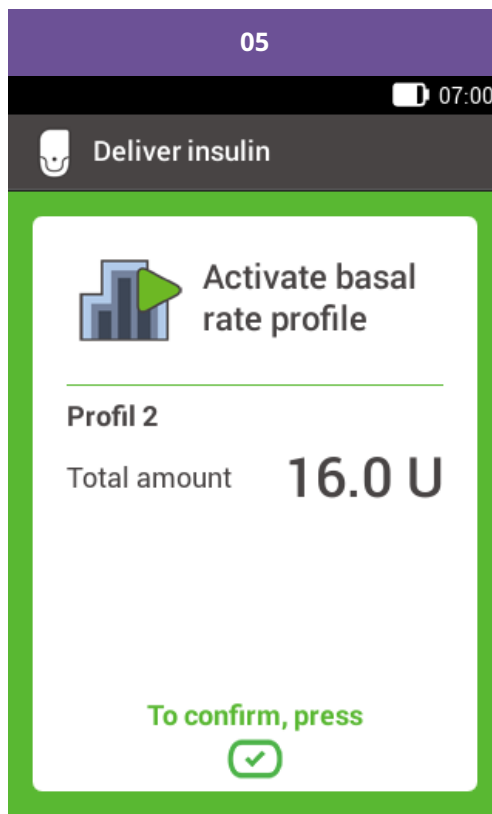

To confirm, press the insulin button .



Changing a basal rate profile

01


Basal rate profiles

Profile 1
Total amount 12.0 U

Profile 2
Total amount 16.0 U

To add a new basal rate profile, tap "+".

Tap the basal rate profile you want to change (for example, Profile 2).

The currently active basal rate profile is indicated by .

02

Basal rate profile

Profil 2

Start	End	U/h
07:00	08:30	1.50
08:30	09:00	1.30
09:00	10:00	0.90

Save Activate

Tap an end time to change the end time for the time block.


Tap a basal rate to change the basal rate for the time block.

Repeat this process until the correct basal rate has been programmed for all 24 hours of the day.

Tap **Save**.

Note

If required, scroll the screen upwards to be able to check all time blocks of the basal rate profile.

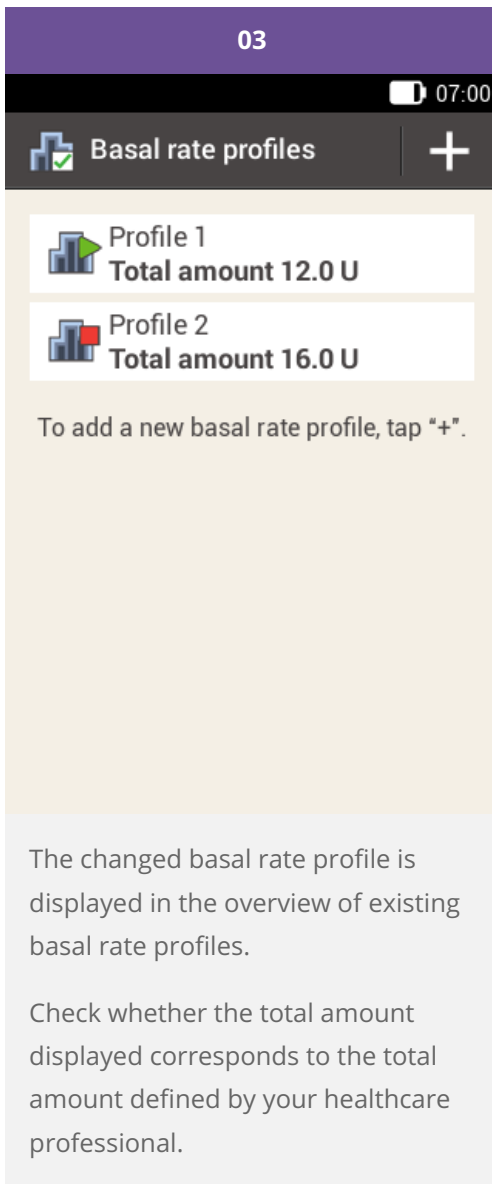

Deleting a basal rate profile

01

07:00

5.9 mmol/L
06:55, 29 Mar 2018

150 U

Profile 1
1.20 U/h

New bolus +

Main menu Add data

07:00

Bolus Basal rate Stop

Test Replace Settings



My data Connect Flight mode


Signals Help


Status screen Add data


On the Status screen, tap the basal rate profile.

On the main menu, tap Basal rate.

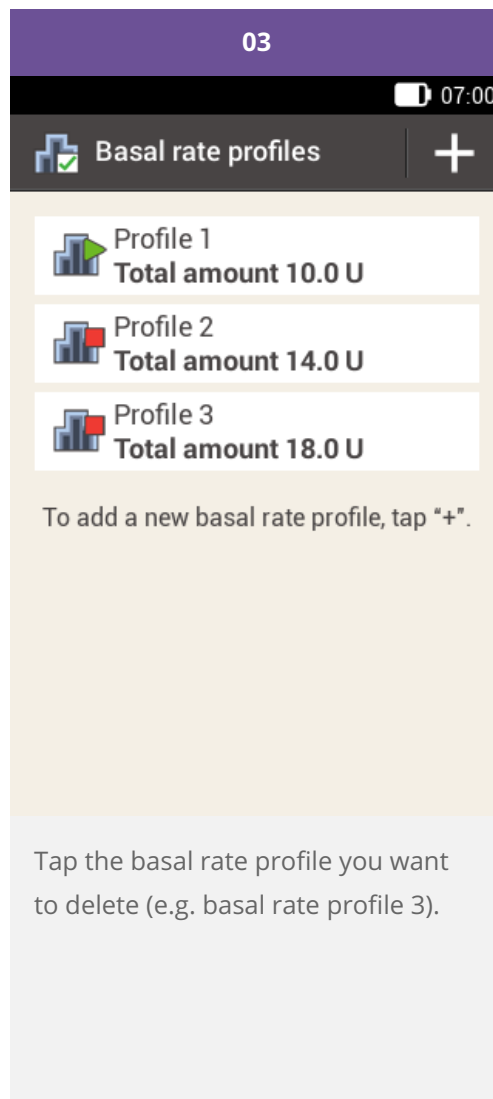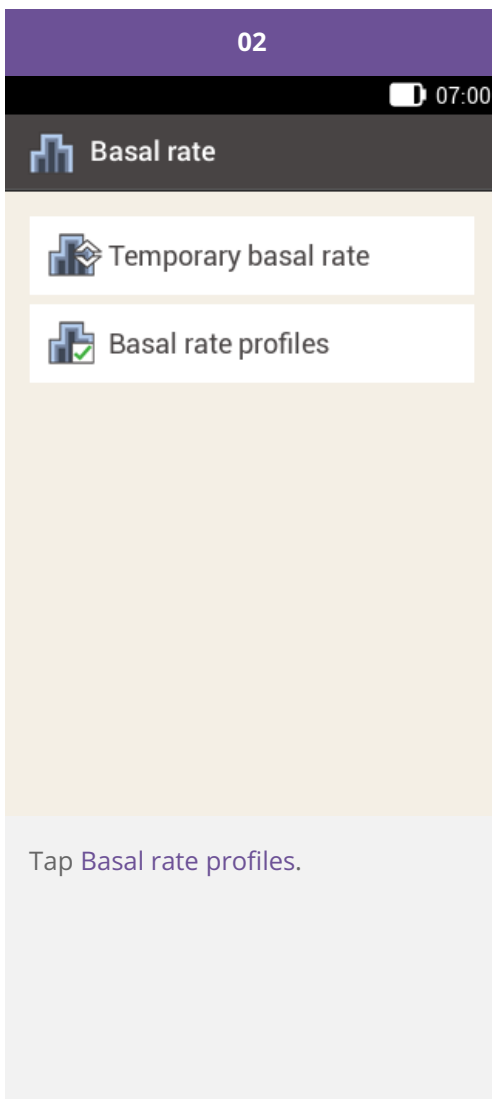

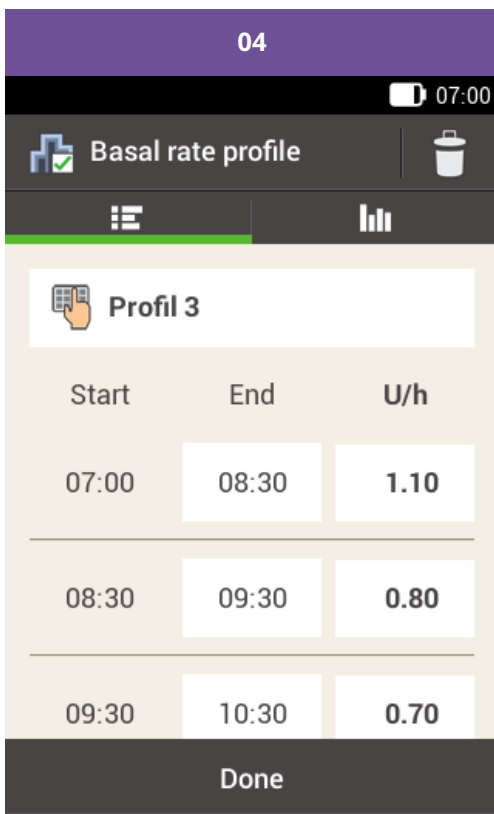

Tap  in the right upper corner of the screen.

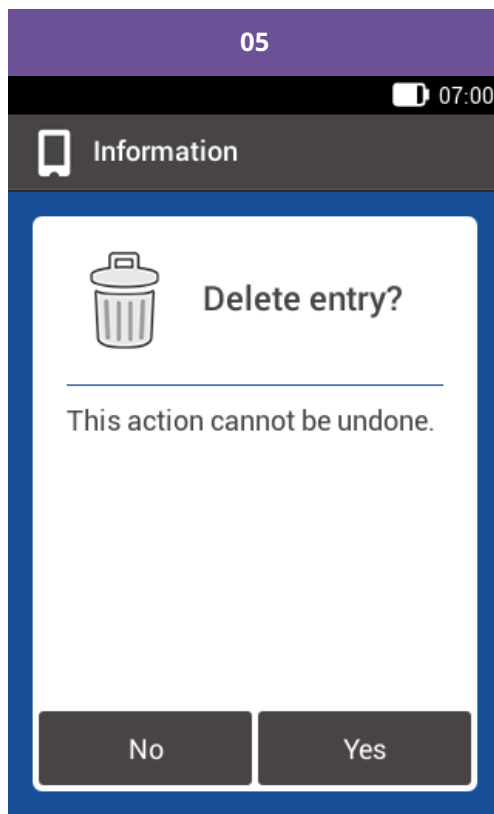

If the active basal rate profile is to be deleted, the following display appears.

Tap Yes.



Basal rate profiles



Profile 1

Total amount 10.0 U

Profile 2

Total amount 14.0 U

To add a new basal rate profile, tap "+".

The selected basal rate profile has been deleted from the list.

Approved/listed/registered under the product name:
Accu-Chek Solo micropump system

ACCU-CHEK, ACCU-CHEK AVIVA, ACCU-CHEK AVIVA SOLO, ACCU-CHEK
SMART PIX,
ACCU-CHEK SOLO and FASTCLIX are trademarks of Roche.

The Bluetooth® word mark and logos are registered trademarks owned by
Bluetooth SIG,
Inc. and any use of such marks by Roche is under license.

All other product names and trademarks are the property of their
respective owners.

© 2021 Roche Diabetes Care

Roche Diabetes Care GmbH
Sandhofer Strasse 116
68305 Mannheim, Germany
www.accu-chek.com

